

# Evaluation of two computer-aided design software on the adaptation of digitally constructed maxillary complete denture

Eman G. Abd El Galil, Shaimaa L. Mohamed<sup>1</sup>, Fardos N. Rizk, Marwa E. Sabet

Department of Removable Prosthodontics, Faculty of Dentistry, The British University in Egypt, <sup>1</sup>Department of Removable Prosthodontics, Faculty of Dentistry, Ain Shams University, Cairo, Egypt

## Abstract

**Aims:** This study was conducted to evaluate the adaptation of maxillary complete denture designed by two different open computer-aided design software programs (3Shape and Exocad) using Geomagic surface matching software.

**Settings and Design:** This was a nonrandomized crossover clinical trial.

**Materials and Methods:** Twenty completely edentulous patients were selected in this study. Forty complete dentures were designed using two different software programs: twenty dentures were designed by 3Shape software and the other twenty dentures were designed by Exocad software. Maxillary dentures were evaluated regarding their adaptation by measuring the deviations that occurred between the fitting surface of the three-dimensional printed dentures, and the scanned master casts using Geomagic surface matching software.

**Statistical Analysis Used:** An unpaired *t*-test was used for statistical analysis.

**Results:** According to the positive average deviation value that represented pressure areas, 3Shape-designed maxillary dentures showed significantly lower mean deviation values ( $0.041115 \pm 0.018165$  mm) than Exocad-designed maxillary dentures ( $0.500665 \pm 0.032619$  mm). Regarding the negative average deviation values that represented the gap areas, Exocad-designed maxillary dentures showed significantly lower mean deviation values ( $0.161555 \pm 0.007842$  mm) than 3Shape-designed maxillary dentures ( $0.231350 \pm 0.009146$  mm). The results of the total average deviation values showed significantly lower mean deviation values ( $0.096950 \pm 0.008868$  mm) of 3Shape-designed maxillary dentures than Exocad-designed maxillary dentures ( $0.250755 \pm 0.021154$  mm).

**Conclusion:** 3Shape and Exocad software programs produced acceptable maxillary dentures regarding denture adaptation. However, maxillary dentures designed by 3 Shape software showed better adaptation than maxillary dentures designed by Exocad software.

**Keywords:** 3Shape software, computer-aided design, denture adaptation, digital complete dentures, Exocad software, Geomagic software

**Address for correspondence:** Dr. Eman G. Abd El Galil, The British University in Egypt, Cairo, Egypt.

E-mail: [eman.khedr@bue.edu.eg](mailto:eman.khedr@bue.edu.eg)

**Submitted:** 10-Apr-2021, **Revised:** 07-Aug-2021, **Accepted:** 15-Sep-2021, **Published:** 09-Nov-2021

Access this article online	
Quick Response Code: 	Website: <a href="http://www.j-ips.org">www.j-ips.org</a>
	DOI: <a href="https://doi.org/10.4103/jips.jips_137_21">10.4103/jips.jips_137_21</a>

This is an open access journal, and articles are distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 4.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as appropriate credit is given and the new creations are licensed under the identical terms.

**For reprints contact:** [WKHLRPMedknow\\_reprints@wolterskluwer.com](mailto:WKHLRPMedknow_reprints@wolterskluwer.com)

**How to cite this article:** El Galil EG, Mohamed SL, Rizk FN, Sabet ME. Evaluation of two computer-aided design software on the adaptation of digitally constructed maxillary complete denture. *J Indian Prosthodont Soc* 2021;21:383-90.

## INTRODUCTION

The conventional complete denture is considered the gold standard in treating completely edentulous patients, but unfortunately, this conventional protocol requires multiple patient visits, in addition to a long laboratory time. Nowadays, complete dentures can be constructed using the traditional method, and be simplified by computer programs, not only to decrease the number of patients visit but also to produce a very efficient complete denture.<sup>[1]</sup>

In the 1990s, Maeda *et al.*<sup>[2]</sup> fabricated a complete denture for the first time by using computer-aided design/computer-aided manufacturing (CAD/CAM) technology. It was made from photo-polymerized composite resin material with the help of a rapid prototyping technique, which is three-dimensional (3D) laser lithography.

All commercially available systems for complete dentures can receive the standard tessellation language (STL) files whether these files are cast scans, impression scans, or even intraoral scans.<sup>[3-5]</sup>

A digital denture could be designed using few commercial CAD software closed systems such as Avadent software (Global Dental Science Scottsdale, AZ, USA), and Dentca software (Dentca Inc, CA, USA), while 3Shape (3Shape, Copenhagen, Denmark), Exocad software (Exocad GmbH, Germany), DWOS full denture (Dental wings by Straumann, Germany) and Bluesky software (Bluesky Bio) are open systems..<sup>[6-10]</sup>

Concerning the accuracy and the precision of digital denture fabrication, the digital denture accuracy and precision are greater than the conventional methods. This accuracy will affect denture retention, stability, and denture fit.<sup>[10-12]</sup> It is predicted that after several years, the digital denture will be the conventional treatment due to its speed, accuracy, treatment quality, patients' satisfaction, and comfort.<sup>[13,14]</sup>

Thus, this study was prompted to evaluate which open system software program whether 3Shape or Exocad produces more adapted maxillary denture.

## MATERIALS AND METHODS

### Study design

This was a nonrandomized crossover clinical trial.

### Patient selection

Twenty completely edentulous patients with a mean age of 60 years old were selected with the following inclusion criteria: completely edentulous patients for at

least 6 months ago, patients with well-developed ridges of different sizes and shapes, and patients having Class I maxillomandibular relationship. Patients with inflamed mucosa, flabby ridge, and undergoing chemotherapy or radiotherapy were excluded. The period of this study started from March 2019 to February 2021. No follow-up period was needed. This research was approved by the Research ETHICS Committee, Faculty of dentistry, Ain Shams University and with code: FDASU-Rec ID021909.

All patients were informed in detail about the nature and period of the investigation, in addition to the purpose of the study. Each patient was informed about the clinical and laboratory procedures of this study, they agreed to take part in the study, knew their legal duties toward this study, and signed on informed consent. All participants were informed about their legal rights for having the best-adapted denture at the end of this study. Guidelines were followed according to the ethical committee of the institution for clinical trials.

For all patients, primary impressions were taken using alginate impression material (Cavex, Holland) in a properly selected and modified stock tray, then poured in dental stone (Durguix, hard natural stone, Spain) to obtain preliminary casts. Self-cured acrylic resin trays (Cold cured acrylic resin, Acrostone, Egypt) were constructed and used to take secondary impressions with rubber base material (Speedex, Coltene, Whaledent AG, Switzerland). Secondary impressions were boxed, then poured in dental stone to obtain the master cast. Occlusion blocks were constructed using self-cured acrylic resin (Cold cured acrylic resin, Acrostone, Egypt) and wax rims (Cavex wax, The Netherlands, Holland) to record the jaw relation using the check bite registration technique.

### Grouping of the study

A total of forty complete dentures were constructed:

- Group A: Twenty maxillary and mandibular complete dentures were designed by 3Shape software
- Group B: Twenty maxillary and mandibular complete dentures were designed by Exocad software.

### Data acquisition

Master casts with jaw relation records of the patients were scanned using 3Shape D850 scanner (D850, 3Shape, Copenhagen, Denmark) to have a total number of twenty scanned master cast and twenty scanned jaw relation records. The STL files were imported to the selected software.

### Computer-aided design

Forty dentures were designed by two different software programs: 3Shape software program (3Shape dental





**Figure 2:** Final design of Exocad denture

new files for the supported denture bases and the teeth was done.


The STL file of denture bases with the supporting arms was sent to the same 3D printer filled with pink denture base printing resin (NextDent, Denture 3+, Netherlands). The STL file of denture teeth with the supporting arms was sent to the same 3D printer filled with white teeth printing resin (NextDent teeth, Netherlands). The printing resin was the same for both dentures.

Finishing of the denture bases and denture teeth was done by removing the support arms by carbide disc, then they were rinsed in alcohol. Minimum polishing was made to them. The teeth were attached to the denture base by fitting them in the teeth recess in the denture bases. The excess resin of both denture bases and denture teeth was used to attach them together. The complete dentures were cleaned, dried, and placed in the postcuring unit (Mogassam, Egypt) for 15 min.

### Denture adaptation evaluation

The fitting surface of the maxillary dentures was sprayed, scanned, and flipped to resemble a cast surface then was saved as an STL file [Figure 5].

Geomagic software (Geomagic Control X 64, 3D systems) was used to evaluate the adaptation of the maxillary denture bases of both the groups. The master cast STL file was selected as reference data, and the STL file of the flipped fitting surface of the denture was selected as measured data. Both files were automatically aligned together by selecting the “best-fit alignment” icon.

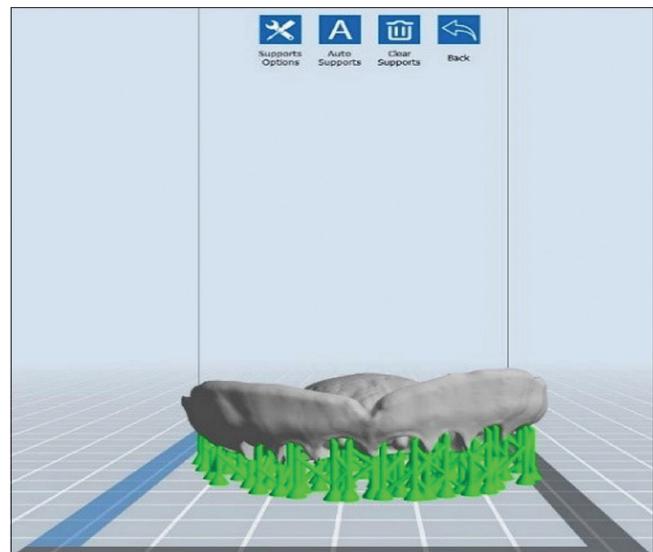

**Figure 3:** Denture bases with the supporting arms on flash print software

The adaptation of the denture bases was automatically generated as a color map according to the distance between the fitting surface of the denture base and the reference data. The cyan to the blue color indicated space between the denture base and the cast surface, the yellow to the red color indicated impingement of the denture base to the cast, and the green color indicated intimate contact between the two surfaces, in addition to the presentation of the denture adaptation as numerical values. The average positive deviation value indicated the pressure areas. The average negative deviation value indicated the gap distance [Figure 6].

The obtained data were recorded, tabulated, and statistically analyzed. The most adapted dentures were delivered to the patients.


### Statistical analysis methods

The sample size was calculated by G\*Power software for windows version 3.1.9.4 assuming a large effect size, a sample size of 20 dentures in each group was calculated to have 95% power,  $\alpha = 0.05$ ,  $1-\beta = 0.95$ .

Statistical analysis was performed with IBM (IBM Corporation, NY, USA) SPSS (SPSS, Inc., an IBM Company) Statistics Version 20 for Windows. An unpaired *t*-test was used for comparison between both groups. The significant level was set at  $P \leq 0.05$ .

### RESULTS

Results of a total of forty maxillary complete dentures: twenty maxillary dentures designed by 3Shape (Group A) and twenty maxillary dentures designed by Exocad (Group B)

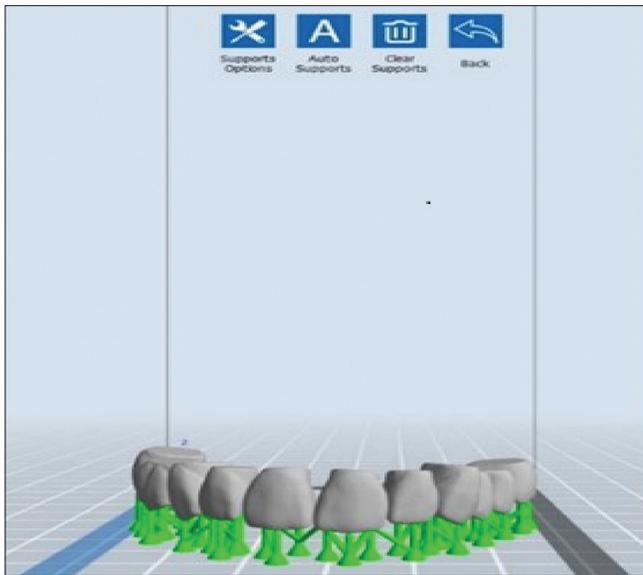

**Figure 4:** Denture teeth with the supporting arms on FlashPrint software

were presented in the form of positive average deviation values (pressure areas), negative average deviation values (gap areas), and total average deviation value.

**Positive average deviation values (pressure areas)**

3Shape-designed maxillary dentures had less positive average deviation from the scanned master cast, so less pressure areas, while Exocad-designed maxillary dentures had higher deviation. This difference was statistically highly significant using an unpaired *t*-test, with a 95% confidence interval from -0.106411 to -0.072609 [Table 1].

**Negative average deviation values (gap areas)**


Exocad-designed maxillary dentures had less negative average deviation from the scanned master cast, so less gap areas, while 3Shape-designed maxillary dentures had higher deviation. This difference was statistically highly significant using an unpaired *t*-test, with a 95% confidence interval from 0.064342 to 0.075248 [Table 2].

**Total average deviation values**

Regarding total average deviation values, 3Shape-designed maxillary dentures had less deviation from the scanned master cast, so better adaptation, while Exocad-designed maxillary dentures had higher deviation. This difference was statistically highly significant using an unpaired *t*-test, with a confidence interval from -0.164188 to -0.143422 [Table 3].

**DISCUSSION**

The main approach for this study was to evaluate which software program will produce the most adaptable denture since adequate denture adaptation will result in good retention, stability, and support.<sup>[15]</sup>

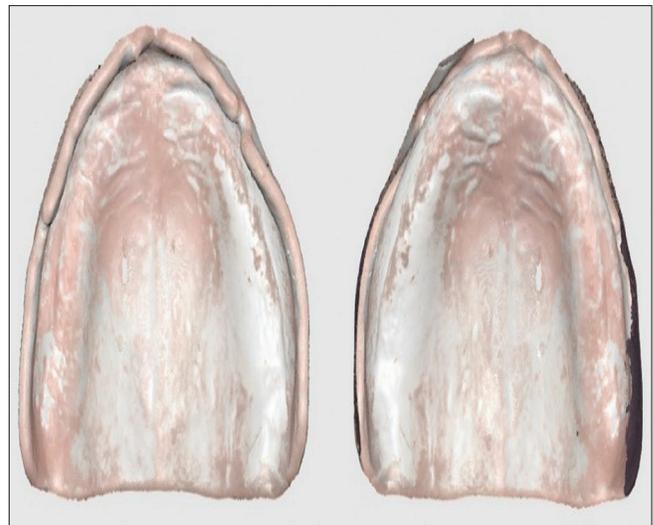

**Figure 5:** The scanned and the flipped fitting surface of the denture

**Table 1: Mean, standard deviation, and P value of unpaired t-test of the positive average deviation values of the denture adaptation (pressure areas) of two groups**

Denture adaptation: Positive average values (pressure area), mean±SD		
3Shape-designed maxillary dentures	Exocad-designed maxillary dentures	P
0.0411155±0.018165	0.500665±0.032619	≤0.0001*

\*Highly significant at  $P \leq 0.0001$ . SD: Standard deviation

**Table 2: Mean, standard deviation, and P value of unpaired t-test of the negative average deviation values of the denture adaptation (gap areas)**

Denture adaptation: Negative average values (gap area), mean±SD		
3Shape-designed maxillary dentures	Exocad-designed maxillary dentures	P
0.231350±0.009146	0.161555±0.007842	≤0.0001*


\*Highly significant at  $P \leq 0.0001$ . SD: Standard deviation

**Table 3: Mean, standard deviation, and P value of unpaired t-test of the total average deviation values of the denture adaptation**

Denture adaptation: Total average deviation, mean±SD		
3Shape-designed maxillary dentures	Exocad-designed maxillary dentures	P
0.096950±0.008868	0.250755±0.021154	≤0.0001*

\*Highly significant at  $P \leq 0.0001$ . SD: Standard deviation

Patients were selected to obtain the data of this study; this ensures the real results of having master casts with different residual alveolar ridge shapes and sizes. However, any available anatomical factor for a specific patient will not affect the results of the study as it is a crossover study. Patients having Class I maxillomandibular relationships were selected for standardization and easily recording the jaw relation.<sup>[16-18]</sup> No control group was made since a control group will require a conventional maxillary complete

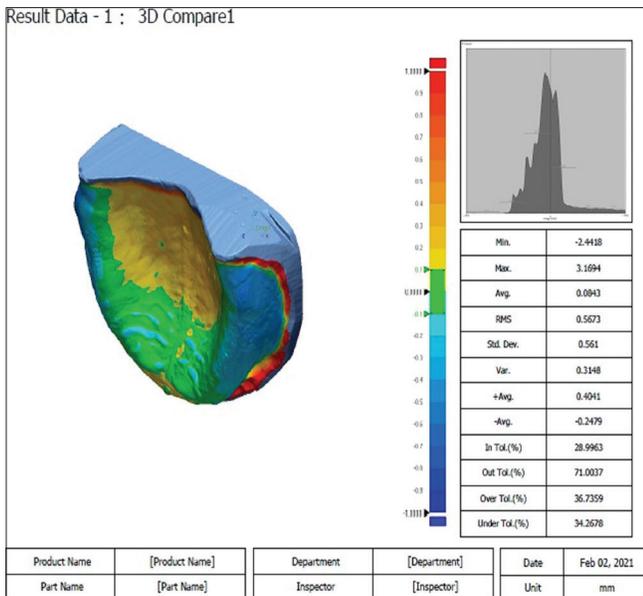

**Figure 6:** Results of three-dimensional comparison were generated as Geomagic report

denture processed by manual techniques with different material; therefore, it will not be standardized.

The operator who designed the dentures was different from the operator who assessed and evaluated the adaptation of the constructed denture. Patients' data were also coded by a third person to ensure the blindness of the assessor.

CAD software evolution allowed the digitalization of complete dentures which allowed for CAM of either the denture bases or the artificial teeth. 3Shape and Exocad software programs are the most popular CAD software programs used in digital dentistry with an open-source license, both software programs have similar designing steps, also these programs allow the operator to import any STL file and export it to any manufacturing machine whether a 3D printer or milling machine, unlike the closed systems that only allow their exported files to be manufactured through their machines.<sup>[19-22]</sup>

Although 3Shape and Exocad software programs accept intraoral scanning, in this study, the desktop scanner was used to scan the master casts and jaw relation records instead of the intraoral scanner because till now, the intraoral camera does not accurately record the functional depth of the vestibules, especially in the mandibular ridges.<sup>[23,24]</sup>

Adaptation is defined as the degree of fit between a prosthesis and supporting structures.<sup>[25]</sup> Adaptation measurements were performed on maxillary ridges since they have better surface area than the mandibular ridges,

so this allows Geomagic software to detect easily several anatomical points for automatic alignment between the measured and the reference data using “best fit alignment” to generate the report of the denture adaptation which gives a realistic result.<sup>[26]</sup>

The adaptation of the denture bases is interpreted as a color map according to the distance between the fitting surface of the denture base and the reference data. The cyan to the blue color indicated space between the denture base and the cast surface, the yellow to the red color indicated impingement of the denture base to the cast, and the green color indicated intimate contact between the two surfaces. The denture adaptation was also presented as numerical values. The average positive deviation value indicated pressure areas and the average negative deviation value indicated the gap distance. This method was in accordance with several studies.<sup>[27-31]</sup>

In this study, the positive average deviation values for 3Shape- and Exocad-designed dentures were  $0.411155 \pm 0.018165$  and  $0.500665 \pm 0.032619$  mm, respectively, while the negative average deviation values of 3Shape- and Exocad-designed dentures were  $0.231350 \pm 0.009146$  and  $0.161555 \pm 0.001754$  mm, respectively. Regarding the total average deviation values of 3Shape-designed dentures and Exocad-designed dentures were  $0.096950 \pm 0.008868$  and  $0.250755 \pm 0.021154$  mm respectively. The results are consistent with the study of You *et al.*<sup>[32]</sup> which stated that the negative average deviation values were  $0.299 \pm 0.035$  mm, also it was consistent with the study of Kalberer *et al.*<sup>[33]</sup> which stated that the total average deviation values were  $0.0953 \pm 0.0075$  mm, while Russo *et al.*<sup>[30]</sup> stated that the total average deviation values were  $0.018 \pm 0.021$  mm. While Hwang *et al.*<sup>[34]</sup> conducted a study stated that the positive average deviation values were  $0.0632 \pm 0.004$  mm, while the negative average deviation values were  $0.063 \pm 0.005$  mm, and the total average deviation values were  $<0.1$  mm.

The results of this study showed that each software program was capable of producing dentures with superior adaptation since it is considered that the acceptable range for the adaptation deviation is 0.05 mm up to 0.3 mm.<sup>[16,34,35]</sup> However, these differences in the results between the two software programs might be due to that 3Shape software had easier steps and fewer number of designing steps, especially the steps of the model analysis, unlike Exocad software that required multiple design steps, which might lead to progression of errors. The increased number of steps of model analysis needs prolonged computational time that might lead to decreased focus, especially with

a less experienced operator. This was in addition to the compatibility between the 3Shape software and its scanner, where there is no Exocad scanner available in the market.

### Clinical implication

This study helps operators to select the most suitable software program in their clinic for designing complete dentures.

### Limitations

- The evaluation of adaptation was performed extra-orally, so the dynamic feature of the soft tissues during mastication cannot be assessed
- This study compared only the maxillary complete dentures, not the mandibular ones.

### Recommendation

- Clinical evaluation for adaptation of maxillary complete dentures is recommended
- Adaptation of the digital maxillary complete dentures is recommended to be evaluated using other types of scanners instead of 3Shape desktop scanners
- Evaluation of adaptation of mandibular complete denture is recommended.

### CONCLUSIONS

Both the software programs produced acceptable maxillary complete dentures regarding denture adaptation. However, maxillary complete dentures designed by 3Shape software showed better adaptation than maxillary complete dentures designed by Exocad software.

### Financial support and sponsorship

Nil.

### Conflicts of interest

There are no conflicts of interest.

### REFERENCES

1. Kattadiyil MT, AlHelal A, Goodacre BJ. Clinical complications and quality assessments with computer-engineered complete dentures: A systematic review. *J Prosthet Dent* 2017;117:721-8.
2. Maeda Y, Minoura M, Tsutsumi S, Okada M, Nokubi T. A CAD/CAM system for removable denture. Part I: Fabrication of complete dentures. *Int J Prosthodont* 1994;7:17-21.
3. Russo L, Salamini A, Troiano G, Guida L. Digital dentures: A protocol based on intraoral scans. *J Prosthet Dent* 2021;125:597-602.
4. Baba NZ, Alrumaih HS, Goodacre BJ, Goodacre CJ. Current techniques in CAD/CAM denture fabrication. *Gen Dent* 2016;64:23-8.
5. AlHelal A, AlRumaih HS, Kattadiyil MT, Baba NZ, Goodacre CJ. Comparison of retention between maxillary milled and conventional denture bases: A clinical study. *J Prosthet Dent* 2017;117:233-8.
6. Ma Z, Han W, Iv Y, Li Y, Cao J, Han Y, *et al.* Design of complete dentures by adopting CAD developed for fixed prostheses. *J Prosthodont* 2016;27:212-9.

7. Kattadiyil MT, Goodacre CJ, Baba NZ. CAD/CAM complete dentures: A review of two commercial fabrication systems. *J Calif Dent Assoc* 2013;41:407-16.
8. Su FY, Tsai JC, Morton D, Lin WS. Use of an open-source CAD software program and additive manufacturing technology to design and fabricate a definitive cast for retrofitting a crown to an existing removable partial denture. *J Prosthet Dent* 2019;122:351-4.
9. Lee SY, Kim H, Lee D, Park C. Modified digital workflow for artificial tooth exchange in a complete denture: A dental technique. *J Prosthet Dent* 2020;123:236-8.
10. Kanazawa M, Iwaki M, Arakida T, Minakuchi S. Digital impression and jaw relation record for the fabrication of CAD/CAM custom tray. *J Prosthodont Res* 2018;62:509-13.
11. AlHelal A, Jekki R, Richardson PM, Kattadiyil MT. Application of digital technology in the prosthodontic management of a patient with myasthenia gravis: A clinical report. *J Prosthet Dent* 2016;115:531-6.
12. Goodacre BJ, Goodacre CJ, Baba NZ, Kattadiyil MT. Comparison of denture tooth movement between CAD-CAM and conventional fabrication techniques. *J Prosthet Dent* 2018;119:108-15.
13. Bacali C, Mesaroş A, Ştefania, Năstase V, Constantiniuc M. Particularities of CAD-CAM commercial systems with applicability in the orofacial sphere; digital complete denture. *Health Sport Rehabil Med* 2019;20:22-5.
14. Srinivasan M, Kalberer N, Naharro M, Marchand L, Lee H, Müller F. CAD-CAM milled dentures: The Geneva protocols for digital dentures. *J Prosthet Dent* 2020;123:27-37.
15. Murray MD, Darvell BW. The evolution of the complete denture base. Theories of complete denture retention-a review. Part 1. *Aust Dent J* 1993;38:216-9.
16. Goodacre BJ, Goodacre CJ, Baba NZ, Kattadiyil MT. Comparison of denture base adaptation between CAD-CAM and conventional fabrication techniques. *J Prosthet Dent* 2016;116:249-56.
17. McGarry TJ, Nimmo A, Skiba JF, Ahlstrom RH, Smith CR, Koumjian JH. Classification system for complete edentulism. *J Prosthodont* 1999;8:27-39.
18. Rangarajan V, Gajapathi B, Yogesh P, Ibrahim Mm, Kumar Rg, Karthik P. Concepts of occlusion in prosthodontics: A literature review, Part II. *J Indian Prosthodont Soc* 2016;15:200-5.
19. Schweiger J, Stumbaum J, Edelhoff D, Güth JF. Systematics and concepts for the digital production of complete dentures: Risks and opportunities. *Int J Comput Dent* 2018;21:41-56.
20. Patzelt SB, Vonau S, Stampf S, Att W. Assessing the feasibility and accuracy of digitizing edentulous jaws. *J Am Dent Assoc* 2013;144:914-20.
21. Sun J, Zhang FQ. The application of rapid prototyping in prosthodontics. *J Prosthodont* 2012;21:641-4.
22. Bilgin MS, Baytaroglu EN, Erdem A, Dilber E. A review of computer-aided design/computer-aided manufacture techniques for removable denture fabrication. *Eur J Dent* 2016;10:286-91.
23. Lo Russo L, Salamini A. Removable complete digital dentures: A workflow that integrates open technologies. *J Prosthet Dent* 2018;119:727-32.
24. Goodacre B, Goodacre C. Using intraoral scanning to fabricate complete dentures: First experiences. *Int J Prosthodont* 2018;31:166-70.
25. Driscoll CF, Freilich MA, Guckes AD, Knoernschild KL, McGarry TJ. The glossary of prosthodontic terms. *J Prosthet Dent* 2017;117:e1-105.
26. Yoon SN, Oh KC, Lee SJ, Han JS, Yoon HI. Tissue surface adaptation of CAD-CAM maxillary and mandibular complete denture bases manufactured by digital light processing: A clinical study. *J Prosthet Dent* 2020;124:682-9.
27. Hsu CY, Yang TC, Wang TM, Lin LD. Effects of fabrication techniques on denture base adaptation: An *in vitro* study. *J Prosthet Dent* 2020;124:740-7.
28. Wang C, Shi YF, Xie PJ, Wu JH. Accuracy of digital complete dentures: A systematic review of *in vitro* studies. *J Prosthet Dent* 2020;125:249-56.
29. Jin MC, Yoon HI, Yeo IS, Kim SH, Han JS. The effect of build angle

El Galil, *et al.*: Adaptation of digitally designed maxillary complete denture

- on the tissue surface adaptation of maxillary and mandibular complete denture bases manufactured by digital light processing. *J Prosthet Dent* 2020;123:473-82.
30. Lo Russo L, Guida L, Zhurakivska K, Troiano G, Chochlidakis K, Ercoli C. Intaglio surface trueness of milled and 3D-printed digital maxillary and mandibular dentures: A clinical study. *J Prosthet Dent* 2021:S0022-3913(21)00262-6.
  31. You SM, You SG, Lee BI, Kim JH. Evaluation of trueness in a denture base fabricated by using CAD-CAM systems and adaptation to the socketed surface of denture base: An *in vitro* study. *J Prosthet Dent* 2020:S0022-3913(20)30573-4.
  32. You SG, You SM, Kang SY, Bae SY, Kim JH. Evaluation of the adaptation of complete denture metal bases fabricated with dental CAD-CAM systems: An *in vitro* study. *J Prosthet Dent* 2020;125:479-85.
  33. Kalberer N, Mehl A, Schimmel M, Müller F, Srinivasan M. CAD-CAM milled versus rapidly prototyped (3D-printed) complete dentures: An *in vitro* evaluation of trueness. *J Prosthet Dent* 2019;121:637-43.
  34. Hwang HJ, Lee SJ, Park EJ, Yoon HI. Assessment of the trueness and tissue surface adaptation of CAD-CAM maxillary denture bases manufactured using digital light processing. *J Prosthet Dent* 2019;121:110-7.
  35. Artopoulos A, Juszczak AS, Rodriguez JM, Clark RK, Radford DR. Three-dimensional processing deformation of three denture base materials. *J Prosthet Dent* 2013;110:481-7.